

Appendix A Flushing Anaesthetic Machine in Preparation for Malignant Hyperthermia Patient


Step 1

- Connect 2L bag to patient end of circuit




Step 2

- Select Volume Mode
- Confirm

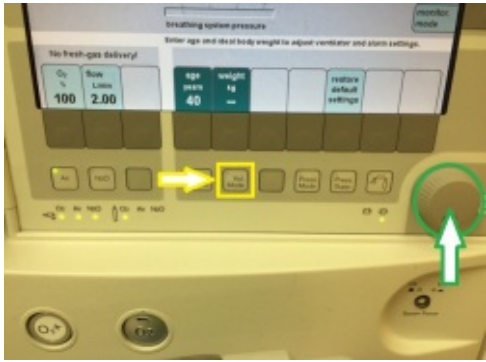

Step 3

- Select Fresh Gas, dial up 18L O<sub>2</sub>
- Confirm

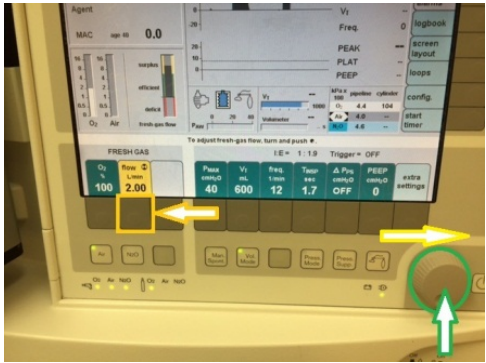

Step 4

- Silence CO<sub>2</sub> Apnea Alarm